



Asian Journal of Pharmaceutical Analysis and Medicinal Chemistry

Journal home page: www.ajpamc.com

<https://doi.org/10.36673/AJPAMC.2020.v08.i04.A16>



A REVIEW ON DEVELOPMENT AND VALIDATION OF HPLC METHOD

Ashish A. Chavan*¹

¹Department of Quality Assurance Techniques, Gourishankar Education Society's Satara College of Pharmacy, Satara, Maharashtra, India.

ABSTRACT

Many extraneous strategies of high-performance liquid chromatographic method development are used today. This review reports a strategy for the systematic development of High-performance liquid chromatographic (HPLC) methods. HPLC is an analytical tool which is effective to detect, separate and quantify the drug, its several impurities and drug related degradants that can form on synthesis or storage. It involves the comprehension of chemistry of drug substance and facilitates the development of analytical method. A number of chromatographic parameters were evaluated in command to optimize the method. An actual mobile phase, column temperature, column, wavelength and gradient must be expert that affords appropriate compatibility and stability of drug as well as degradants and adulteration. Most of the drugs in numerous component dosage forms can be studied by HPLC method because of some advantages like rapidity, specificity, recovery, precision and ease of automation in this method. Validation of HPLC method as per ICH Guidelines protects all the performance characteristics of validation, like Accuracy, precision, specificity, linearity, range and limit of detection, limit of quantification, robustness and system suitability testing.

KEYWORDS

HPLC, Method development and Validation.

Author for Correspondence:

Ashish A. Chavan,
Department of Quality Assurance Techniques,
Gourishankar Education Society's Satara College of
Pharmacy,
Satara, Maharashtra, India.

Email: chavanashish442@gmail.com

INTRODUCTION

High Performance Liquid Chromatography (HPLC) was acquired from the classical column chromatography and, is one of the most important device of analytical chemistry today¹. In the modern pharmaceutical industry, high-performance liquid chromatography (HPLC) is the excellence and important analytical tool applied in all stages of drug discovery, development, and production². HPLC is the method of choice for checking peak

purity of new chemical entities, monitoring reaction changes is in synthetic process or scale up, evaluating new formulations and carrying out quality control / assurance of the final drug products³. The Goal of HPLC method is to try and apart, quantify the main drug, any reaction impurities, all available synthetic intermediates and any degradants⁴. High Performance Liquid Chromatography is now one of the sturdiest tools in analytical chemistry. It has the ability to separate, identify, and quantify the compounds that are present in any sample that can be dissolved in a liquid. HPLC is the most suitable analytical methods generally used for the quantitative as well as qualitative analysis of drug product and used for determining drug product stability⁵. HPLC principle is the solution of sample is injected into a column of porous material (stationary phase) and liquid phase (mobile phase) is pumped at higher pressure through the column. The theory of separation followed is the adsorption of solute on stationary phase based on its affinity towards stationary phase. (Figure No.1) The technique of HPLC has following features⁶.

- High resolution
- Small diameter, Stainless steel, Glass column
- Rapid analysis
- Relatively higher mobile phase pressure
- Controlled flow rate of mobile phase

HPLC Method Development

Methods are expand for new products when unofficial methods are available. Another method for existing (Non-Pharmacopoeia) products are to decrease the cost and time for enhance precision and ruggedness. When another process proposed is calculated to replace the existing procedure relative laboratory data including advantages/disadvantages are made available. The aim of the HPLC-process is to try and separate, quantify the major active drug, any reaction impurities, all available synthetic intermediates and any degradants⁷.

Steps involved in Method development are^{6,7}

- Understanding the Physicochemical properties of drug molecule.
- Set up of chromatographic conditions.

- Developing the approach of analysis.
- Sample preparation
- Method optimization
- Method validation

Understanding the physicochemical properties of drug molecules

Physicochemical properties of an active molecule play an major role in process development. For Method evolution one has to inspect the physical properties like solubility, pKa polarity and pH of the active molecule. Polarity is a physical property of a compound. It assist an interpreter, to determine the solvent and composition of the mobile phase⁶. The solubility of molecules can be explain on the basis of the polarity of molecules. Polar, e.g. water, and nonpolar, e.g. benzene, solvents do not combine. In common, like dissolves like i.e., substance with similar polarity are soluble in each other. Selection of diluents is based on the solubility of test substance. The acidity or basicity of an analyte is defined most commonly by the pH value. Electing a proper pH for ionizable analytes frequently leads to symmetrical and sharp peaks in HPLC⁷.

Set up of chromatographic conditions

Throughout main method evolution, a set of starting conditions (detector, column, mobile phase) is preference to get the first "scouting" chromatograms of the sample. In many cases, these are based on reversed-phase chromatographic separations on a C18 column with UV detection. A conclusion on developing either an isocratic or a gradient method should be made at this point.

Selection of Column

A column is essential to the starting and central part of a chromatograph. A correctly selected column can generate a good chromatographic separation which provides a correct and good analysis. An unsuitable used column can frequently generate confusion, in adequate and bad separations which can lead to results that are invalid or complex to elucidate⁸. The heart of a HPLC system is the column. Changing a column will have the highest effect on the resolution of analytes during process development. Selecting the best column for

application need to consideration of stationary phase chemistry, particle size, retention capacity and column dimensions. The three main part of an HPLC column are the matrix, hardware and the stationary phase. There are different types of matrices for support of the stationary phase, including silica, alumina, polymers and zirconium. Silica is the most usual matrix for HPLC columns. Silica matrices are sturdy, uncomplicated derivative, prepared to compatible sphere size and does not protect to compress under pressure. Silica is chemically stable to most organic solvents and to lower pH systems. One short coming of a silica solid support is that it will liquefy above pH⁷. In current years, silica supported columns have been developed for use at high pH. The separation effected by nature, shape and particle size of silica support. Smaller particle gives a larger number of theoretical plates, or increased. The nature of the stationary phase will establish whether a column can be used for normal phase or reverse phase chromatography. Normal phase chromatography use a polar stationary phase and a non-polar mobile phase. Generally, highly polar compounds elute later than non-polar compounds. Frequently used reverse phase columns and their uses are listed below. Propyl (C3), Butyl (C4) and Pentyl (C5) phases are beneficial for ion-pairing chromatography (C4) and peptides with hydrophobic residues, and extra-large molecules. C3-C5 columns generally retain non-polar solutes more insoluble when compared to C8 or C18 phases. Examples include YMC-Pack C4 and Luna C5. These columns are generally not more stable to hydrolysis than columns with longer alkyl chains. Octyl (C8, MOS) phases have wide applicability. This phase is less retentive than the C18 phases, but is still quite useful for pharmaceuticals, nucleosides, and steroids⁹. Choosing of the stationary phase/column is the first and the most important step in process development. The evolution of a rugged and reproducible method is impossible without the availability of a stable, high performance column. To escape problems from irreproducible sample retention during process development, it is important that columns be stable

and reproducible. The separation selectivity for specific components differ between the columns of various manufacturer as well as between column production batches from the same manufacturer. Column dimensions, silica substrate properties and bonded stationary phase characteristics are the main ones. The use of silica-based packing is favoured in most of the present HPLC columns due to several physical characteristics⁶.

Selection of Chromatographic mode Figure

Chromatographic modes depend on the analyte's molecular weight and polarity. All case reports will focus on reversed-phase chromatography (RPC), the most common mode for small organic molecules. Ionizable substance (acids and bases) are frequently separated by RPC with buffered mobile phases (to keep the analytes in a non-ionized state) or with ion-pairing reagents¹⁰.

Optimization of Mobile phase

Buffer Selection

Various buffers such as sodium phosphate, potassium phosphate and acetate were evaluated for system suitability parameters and overall chromatographic performance.

Effect of pH

If analytes are ionisable, the suitable mobile-phase pH must be select based on the analyte pKa so the target analyte is in one predominate ionization state, ionized or neutral. Renewal of the mobile-phase pH is one of the principal tools in the "chromatographer's toolbox" allowing concurrent change in retention and selectivity between critical pair of components¹¹.

Effect of organic modifier

Choosing of the organic modifier type is relatively simple in reverse phase HPLC, The normal selection is between acetonitrile and methanol (rarely THF). Gradient elution is usually employed with complex multicomponent samples since it may not be possible to get all components eluted between k (retention factor) 1 and 10 using a single solvent strength under isocratic conditions¹¹.

Selection of detector and wavelength

After the chromatographic separation, the analyte of interest is detected by using acceptable detectors. Some commonly used detectors in LC are:

ultraviolet (UV) detectors, electrochemical detectors, fluorescence detectors, refractive index (RI) detectors and mass spectrometry (MS) detectors. The selection of detector depends on the sample and the reason of the analysis. In case of multicomponent analysis, the absorption spectra may have been shifted to longer or shorter wavelengths compared to the parent compound. Therefore, the UV spectra of target analyte and impurities must be taken and overlaid with each other and the spectra should be normalized due to different amounts present in the mixture. A wavelength must be selected such that adequate response is for most of the analytes can be obtained^{11,12}.

Developing the approach for analysis

Even developing the analytical method on RP-HPLC the first step which is followed, the selections of different chromatographic parameters like selection of mobile phase, selection of column, selection of flow rate of mobile phase, selection of pH of mobile phase. All of these parameters are selected on the basis of trials and followed by considering the system suitability parameters. Typical parameters of system suitability are e.g. retention time must be more than 5 min, the theoretical plates must be more than 2000, the tailing factor must be less than 2, resolution between 2 peaks must be more than 5, % R.S.D of the area of analyte peaks in standard chromatograms must not be more than 2.0% like other. Detection wavelength is usually isosbestic point in the case of simultaneous estimation of 2 components⁶.

Sample preparation

Sample preparation is a critical step of process development that the analyst must investigate. For example, the analyst should investigate if centrifugation (determination of the optimal rpm and time) shaking and/or filtration of the sample is needed, particularly if there are insoluble components in the sample. The purpose is to demonstrate that the sample filtration does not influence the analytical result due to adsorption and/or extraction of leachable. The effectiveness of the syringe filters is largely determined by their

ability to evaluate contaminants/insoluble components without leaching undesirable artifacts (i.e., extractable) into the filtrate. The sample preparation method should be adequately described in the respective analytical method that is applied to a real in-process sample or a dosage form for subsequent HPLC analysis. The analytical method must specify the type of filter, manufacturer and pore size of the filter media¹². The motive of sample preparation is to generate a processed sample that leads to better analytical results compared with the initial sample. The prepared sample should be a divide relatively free of interferences that is compatible with the HPLC method and that will not Harm to the column^{12,14}.

Method optimization

Most like of the optimization of HPLC method development has been focused on the optimization of HPLC conditions¹⁴. The mobile phase and stationary phase compositions need to be taken into account. Optimization of mobile phase parameters is always considered is much easier and convenient than stationary phase optimization. To decrease the number of trial chromatograms involved, only the parameters that are likely to have an appreciable effect on selectivity in the optimization must be examined. Primary control variables in the optimization of liquid chromatography (LC) methods are the different components of the mobile phase determining acidity, gradient, solvent, flow rate, sample amounts, injection volume, temperature and diluents solvent type. This is used to find the appropriate balance between resolution and analysis time after satisfactory selectivity has been achieved. The parameters involved column dimensions, column-packing particle size and flow rate. These parameters may be changed without affecting capacity factor or selectivity⁹.

Method Validation

Validation of an analytical method by which it is developed by laboratory studies, that the performance characteristics of the process meet the requirements for the suitable analytical application. Validation is used for any new or revise method to ensure that it is capable of giving reproducible and reliable results, when used by various operators

employing the similar equipment in the same or different laboratories. The type of validation program required depends completely on the particular method and its proposed applications¹². Results of the method validation can be used to judge the quality, reliability and consistency of analytical outcome; it is an integral part of any good analytical practice. Use of equipment that is within adequately calibrated, working correctly and specification is fundamental to the method validation process. Analytical methods need to be validated or revalidated¹⁵.

Before their introduction into routine use;

Whenever the conditions changes the method has been validated

Whenever the method is changed

Particular parameters recommended by FDA, USP and ICH are as follow^{15,17}

Specificity

Linearity and Range

Precision

Method precision (Repeatability)

Intermediate precision (Reproducibility)

Accuracy (Recovery)

Solution stability

Limit of Detection (LOD)

Limit of Quantification (LOQ)

Robustness

System suitability

Specificity

It is an analytical method as its capacity to measure precisely an analyte in the presence of interference, such as synthetic precursors, enantiomers, excipients and known (or likely) degradation products that may be expected to be present in the sample matrix¹⁶.

Linearity and range

The linearity of an analytical method is its strength (within a given range) to produce test results, which are directly proportional to the concentration of analyte in the test solution. A linear relationship should be calculated across the range of the analytical procedure. It is demonstrated directly on the drug particle by dilution of a standard stock solution of the drug product components, using the proposed procedure. Linearity is usually expressed

as the confidence limit around the slope of the regression line¹⁵⁻¹⁷. For the create of linearity, minimum of five concentrations are recommended by ICH guideline¹⁸. The range of an analytical process is the interval between the upper and lower limit that have been express to be determined with precision, accuracy and linearity using the method¹⁶.

Precision

The precision of an analytical method express the degree of agreement within individual test result when method is applied repeatedly to multiple sampling of a homogeneous sample under the prescribed conditions. Precision may be considered at three levels: repeatability, robustness and reproducibility¹⁸. The precision of an analytical process is generally indicate the standard deviation or relative standard deviation of order of measurements. Precision may be also the degree of reproducibility or of the repeatability of the analytical process under standard conditions. Intermediate precision (also known as ruggedness) indicate within laboratories differentiation, as on various days, or with different analysts or instruments within similar laboratory. Precision of an analytical process is decided by analysis an enough number of aliquots of a homogeneous sample to be able to calculate statistically valid evaluates of standard deviation or relative standard deviation¹⁹.

Accuracy (Recovery)

The accuracy of an analytical method indicate the nearness of agreement between the value which is accepted either as a standard true value or an accepted reference value and the value found. It is decided by applying the process to samples to which studied amounts of analyte have been added. These should be examined against standard and blank solutions to secure that no interference exists. The accuracy is then measured from the test results as a percentage of the analyte recovered by the assay. It may frequently be demonstrating the accuracy by the assay of known, added amounts of analyte^{17,18}.

Solution stability

During validation the stability of standards and samples is established under common conditions, common storage conditions, and sometimes in the instrument to determine if special storage conditions are necessary, for illustration, refrigeration or protection from light¹⁷.

Limit of Detection (LOD)

Limit of detection (LOD) of an independent procedure is the lowest amount of analyte in a sample that can be detected but not necessarily quantitated as an exact value. In analytical method that exhibit baseline noise, the LOD can be depending on a signal-to-noise (S/N) ratio (3:1), which is usually shows as the concentration of analyte in the sample. The signal-to-noise ratio is determined by: $s = H/h$ Where H = height of the peak corresponding to the component. h = absolute value of the great noise fluctuation from the baseline of them chromatogram of a blank solution¹⁷⁻¹⁹.

Limit of Quantification (LOQ)

The limit of Quantitation (LOQ) or Quantitation limit of an independent analytical method is the lowest amount of analyte in a sample that can be quantitatively determined with acceptable precision and accuracy. For analytical method such as HPLC that display baseline noise, the LOQ is generally estimated from a determination of S/N ratio (10:1) and is usually confirmed by injecting standards

which give this S/N ratio and have an acceptable percent relative standard deviation as well^{18,19}.

Robustness

Is defined as the measure of the capacity of an analytical process to remain unaffected by small but deliberate variations in process parameters (e.g. pH, mobile phase composition, temperature and instrumental settings) and give an indication of its reliability during normal usage. Determination of robustness is a systematic method of varying a parameter and measuring the effect on the method by monitoring system suitability and/or the analysis of samples^{17,18}.

System Suitability

System suitability tests are an integral part of liquid chromatographic methods. They are used to confirm that the detection sensitivity, resolution and reproducibility of the chromatographic system are sufficient for the analysis to be done. The tests are depends on the concept that the equipment, electronics, analytical operations and samples to be studied constitute a fundamental system that can be estimated as such. Factors, such as the peak resolution, number of theoretical plates, peak tailing and capacity have been measured to determine the applicability of the used method¹⁵⁻¹⁹.

Table No.1: Important Information concerning sample composition and properties

Number of Compounds present
Chemical Structures (functionality) of compounds
Molecular weight of compounds
PKa values of compounds
UV Spectra of compounds
Concentration range of compound in sample of interest Sample Solubility

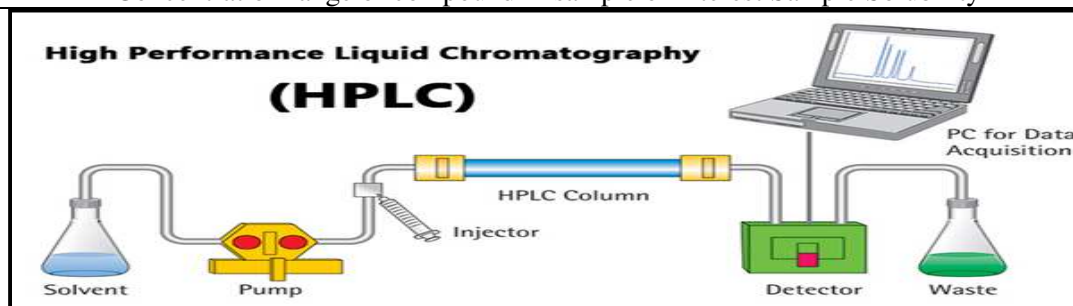


Figure No.1: Flow Diagram of HPLC

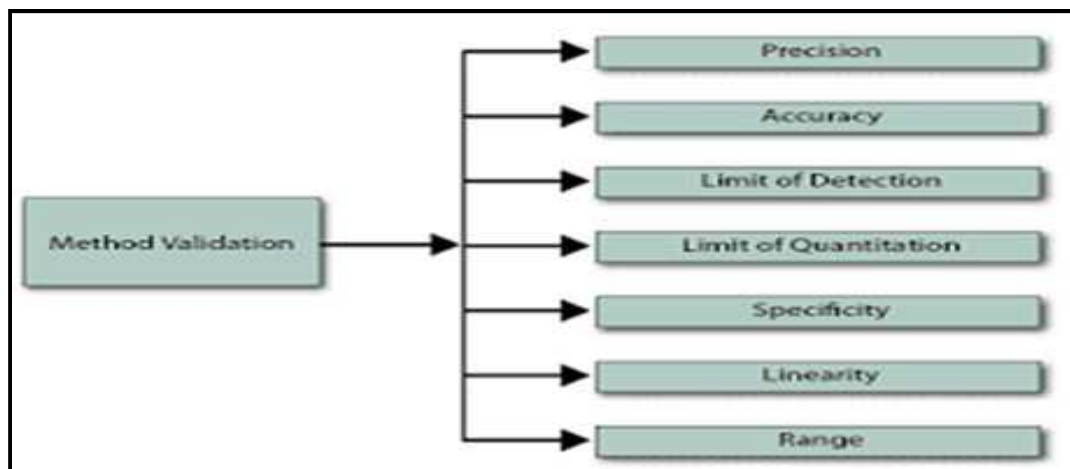


Figure No.2: Method validation parameter

CONCLUSION

In recent years evolution of the analytical methods for identification, purity evaluation and quantification of drugs has received a great deal of attention in the field of pharmaceutical analysis. This review describes HPLC method development and validation in common way. A general and very simple approach for the HPLC method development for the separation of compounds was discussed. Knowledge of the physiochemical properties of the primary compound is of almost importance prior to the any HPLC method development. The choice of buffer and mobile phase composition (organic and pH) plays a dramatic role on the separation selectivity. Final optimization can be performed by altering the gradient slope, temperature and flow rate as well as the type and concentration of mobile-phase modifiers. Optimized method is validated with various parameters (e.g. specificity, precision, recovery, detection limit, linearity, etc.) as per ICH guidelines.

ABBREVIATIONS

HPLC High Performance Liquid Chromatography
 ICH International conference on Harmonization
 Id Internal Diameter
 LC Liquid Chromatography
 LOD Limit of Detection
 LOQ Limit of Quantitation
 m Meter
 mm Mili meter

MS Mass Spectrometry
 ODS Octyl decyl silane
 RI Refractive index
 THF Tetrahydrofuran
 USP United states Pharmacopeia
 μm Micron

ACKNOWLEDGEMENT

The authors wish to express their sincere gratitude to College of Pharmacy, Department of Quality Assurance Techniques, Gourishankar Education Society's Satara College of Pharmacy, Satara, Maharashtra, India for providing necessary facilities to carry out this review work.

CONFLICT OF INTEREST

We declare that we have no conflict of interest.

BIBLIOGRAPHY

1. Gupta V, Jain A D K, Gill N S, Gupta K. Development and validation of HPLC method - A review, *Int. Res J Pharm. App Sci*, 2(4), 2012, 17-25.
2. Kazakevich Y, Lobrutto R. HPLC for Pharmaceutical Scientists, *John Wiley and Sons, New Jersey*, 1st Edition, 2007, 1140.
3. Ahuja S, Rasmussen H. Development for Pharmaceuticals, *Separation Science and Technology, Elsevier, New York*, 1st Edition, 8, 2007, 532.

4. Azim M S, Mitra M, Bhasin P S. HPLC method development and validation: A review, *Int. Res. J. Pharm*, 4(4), 2013, 39-46.
5. Rao B V, Naga Sowjanya G, Ajitha A, Rao V U M. Review on stability indicating HPLC method development, *World Journal of Pharmacy and Pharmaceutical Sciences*, 4(8), 2015, 405-423.
6. Charde M S, Welankiwar A S, Kumar J. Method development by liquid chromatography with validation, *International Journal of Pharmaceutical Chemistry*, 4(2), 2014, 57-61.
7. Sood S, Bala R, Gill N S. Method development and validation using HPLC technique - A review, *Journal of Drug Discovery and Therapeutics*, 2(22), 2014, 18-24.
8. Singh P K, Pande M, Singh L K, Tripathi R P. Steps to be considered during method development and validation for analysis of residual solvents by gas chromatography, *Int. Res J Pharm. App Sci*, 3(5), 2013, 74-80.
9. Prathap B, Rao G H S, Devdass G, Dey A, Harikrishnan N. Review on stability indicating HPLC method development, *International Journal of Innovative Pharmaceutical Research*, 3(3), 2012, 229-237.
10. Dong M W. Modern HPLC for practicing scientists, *John Wiley and Sons, New Jersey*, 2006, 1-30.
11. Kaushal C K, Srivastava B. A process of method development: A chromatographic approach, *J. Chem. Pharm. Res*, 2(2), 2010, 519-545.
12. Toomula N, Kumar A, Kumar S D, Bheemidi V S. Development and validation of analytical methods for pharmaceuticals, *J Anal Bioanal Techniques*, 2(5), 2011, 1-4.
13. Kardani K, Gurav N, Solanki B, Patel P, Patel B. RP-HPLC method development and validation of gallic acid in polyherbal tablet formulation, *Journal of Applied Pharmaceutical Science*, 3(5), 2013, 37-42.
14. Nigovic B, Mornar A, Sertic M. Chromatography - The most versatile method of chemical analysis, *Intech*, 2012, 385-425.
15. Bhagyasree T, Injeti N, Azhakesan A, Rao U M V. A review on analytical method development and validation, *International Journal of Pharmaceutical Research and Analysis*, 4(8), 2014, 444-448.
16. Shrivastava A, Gupta V B, HPLC: Isocratic or gradient elution and assessment of linearity in analytical methods, *J Adv Scient Res*, 3(2), 2012, 12-20.
17. Kumar V, Bharadwaj R, Gaurav Gupta, Kumar S. An overview on HPLC method development, optimization and validation process for drug analysis, *The Pharmaceutical and Chemical Journal*, 2(2), 2015, 30-40.
18. Validation of analytical procedures: Text and methodology, *International Conferences on Harmonization, Q2 (R1)*, 2005.
19. Validation of compendial procedures, *United State Pharmacopeia, USP 36 NF*, 27(2), 2010.
20. Sriguru B, Nandha N P, Vairale A S, Sherikar A V, Nalamothu V. Development and validation of stability indicating HPLC method for the estimation of 5-Fluorouracil and related substances in topical formulation, *Int. J. Res. Pharm. Sci*, 1(2), 2010, 78-85.

Please cite this article in press as: Ashish A. Chavan. A review on development and validation of HPLC method, *Asian Journal of Pharmaceutical Analysis and Medicinal Chemistry*, 8(4), 2020, 129-136.